

FIG. 1A


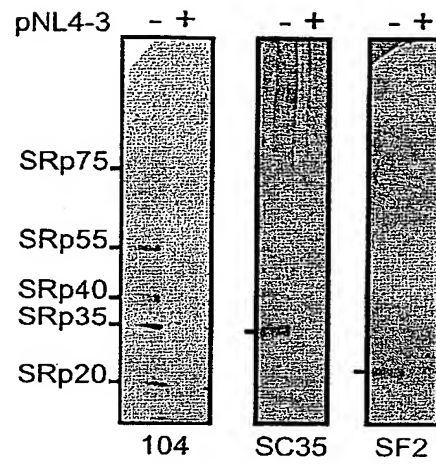


FIG. 1B

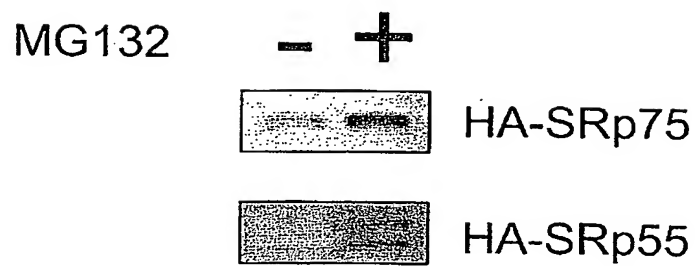

BEST AVAILABLE COPY

FIG. 2A

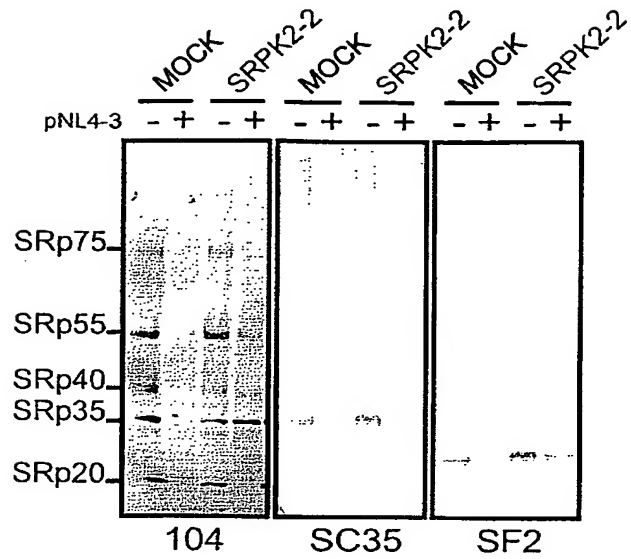


FIG. 2B

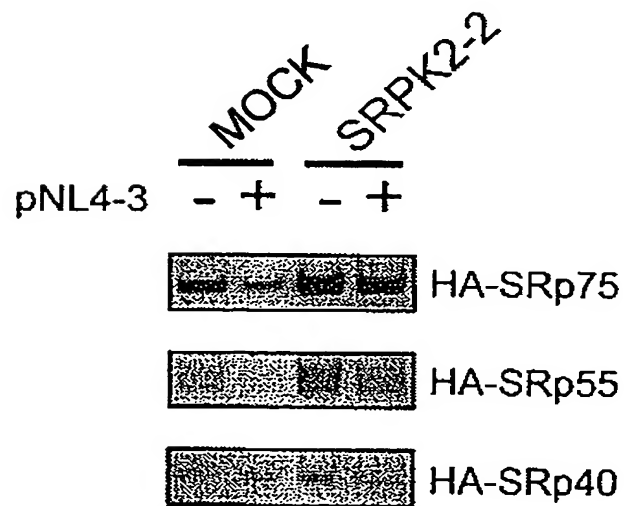


FIG. 2C



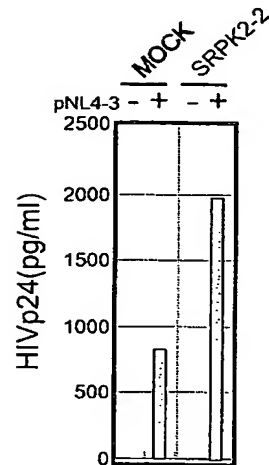


FIG. 3A

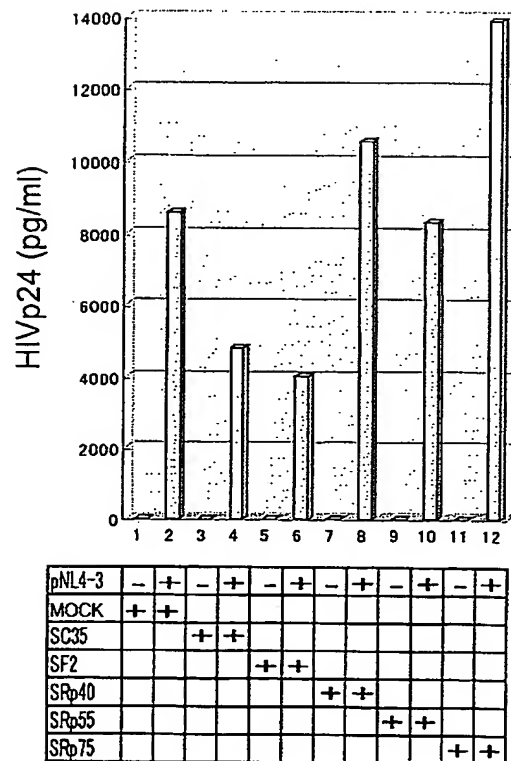


BEST AVAILABLE COPY

FIG. 3B

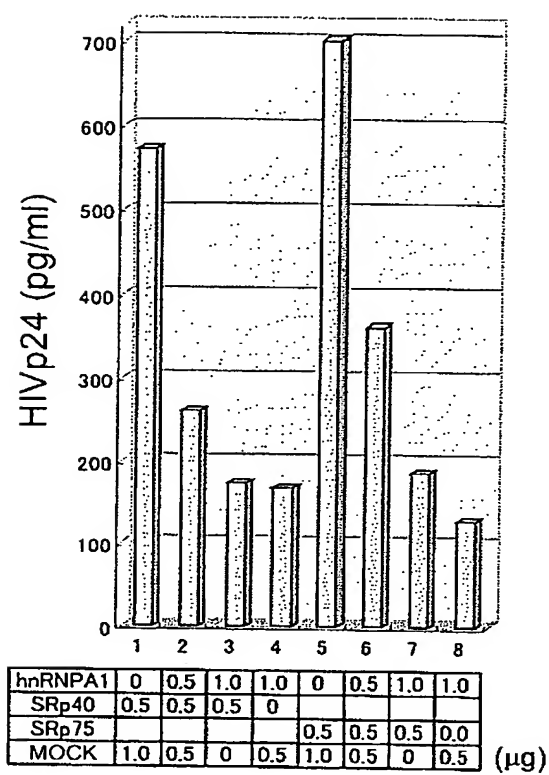


BEST AVAILABLE COPY

FIG. 4A



SRPIN-1(C₁₈H₁₈F₃N₃O)
MW349.35

FIG. 4B

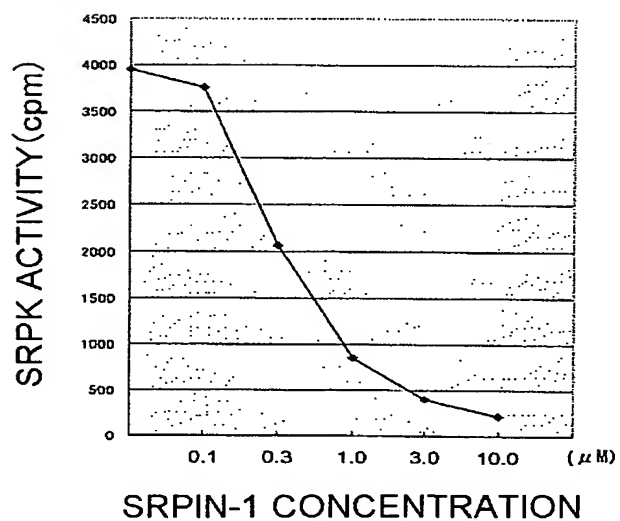

BEST AVAILABLE COPY

FIG. 4C



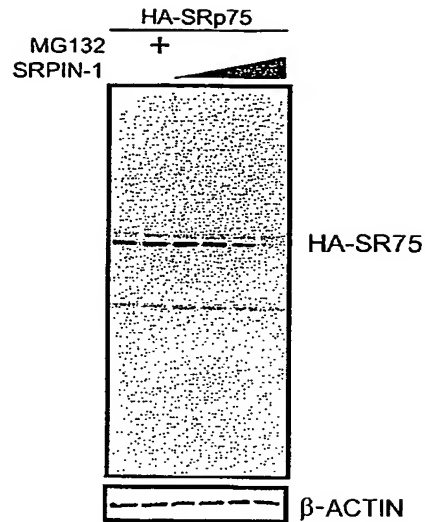


FIG. 4D

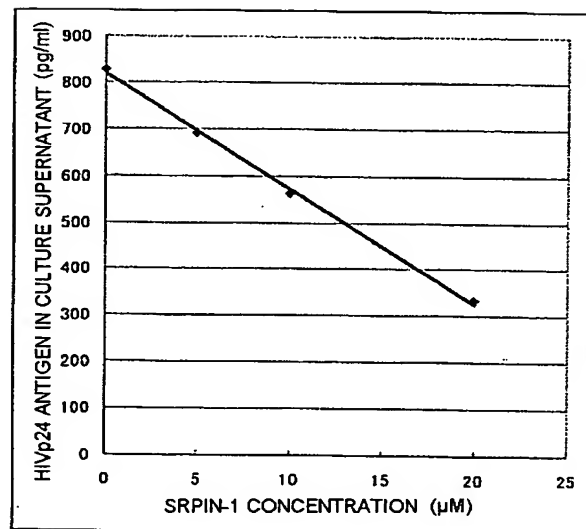

BEST AVAILABLE COPY

FIG. 5A

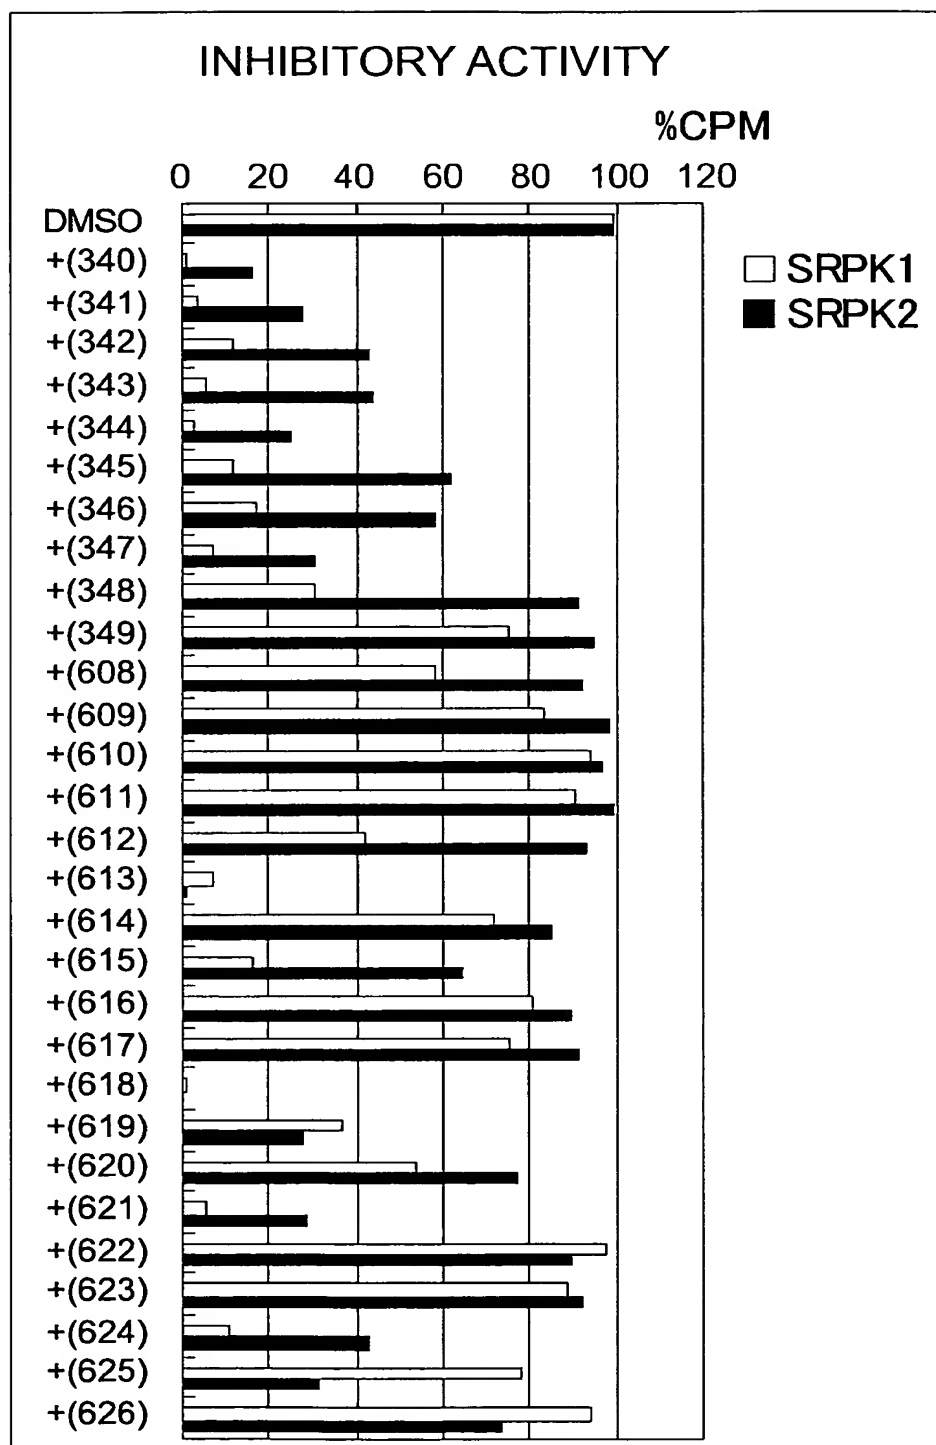

BEST AVAILABLE COPY

FIG. 5B


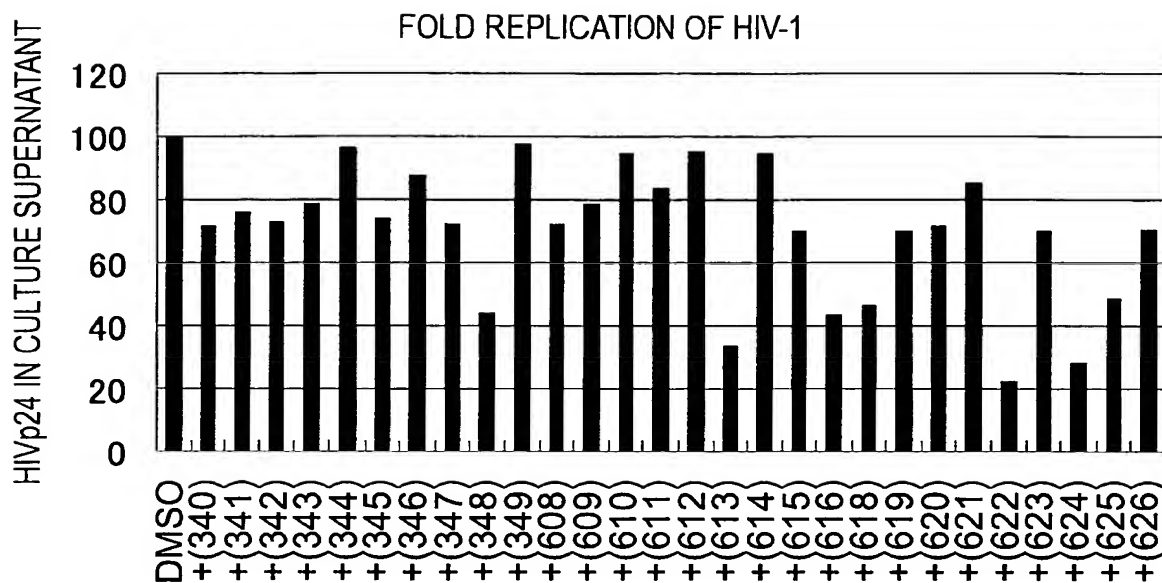


FIG. 5C

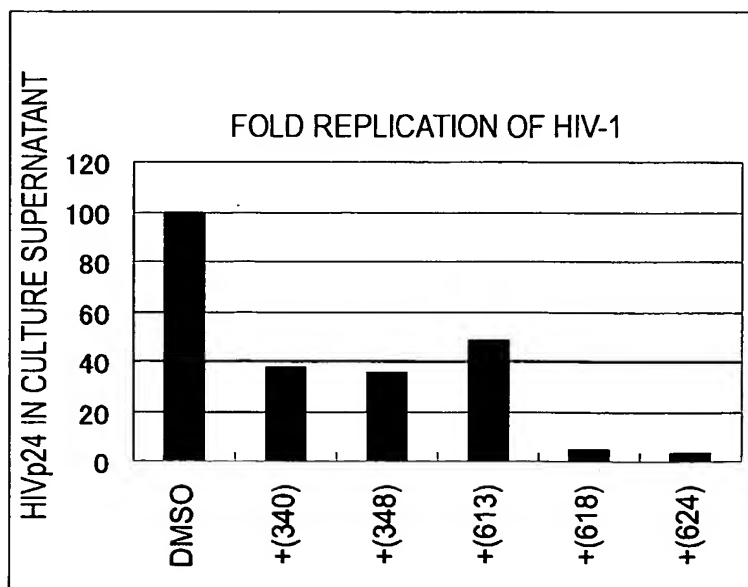

BEST AVAILABLE COPY

FIG. 6A


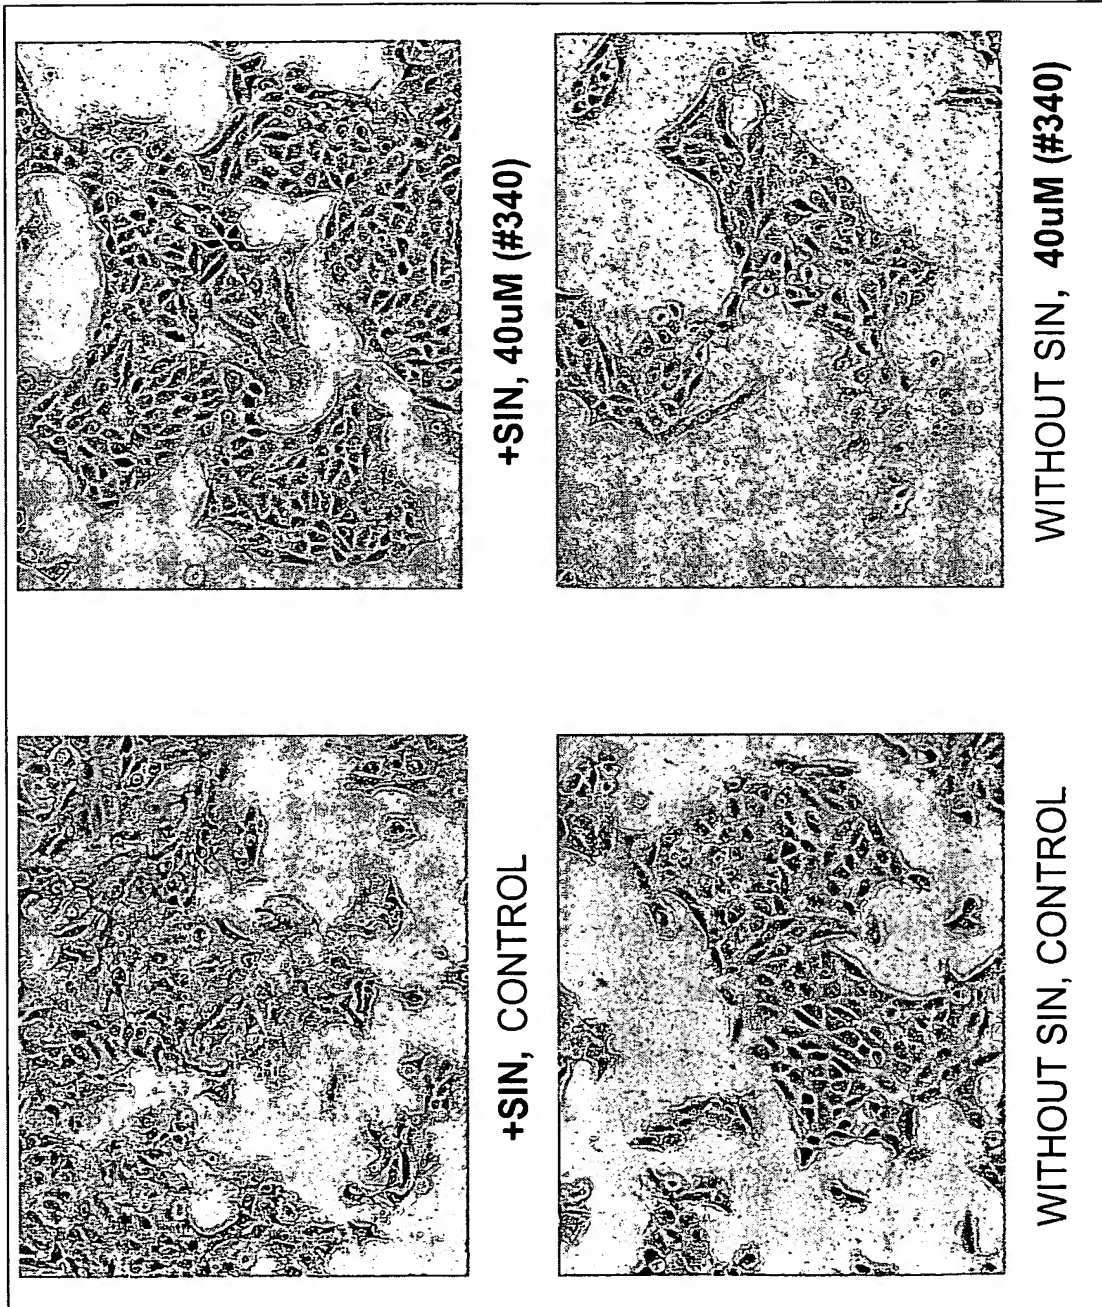


FIG. 6B


PLAQUE ASSAY

RESULTS	N.o	340	PFU/ml	CELL COUNT IN WELL	PLAQUE COUNT
	340c-1	0	1.05×10^7	10^5	21
	340c-2	DMSO	1.20×10^7	10^5	24
	340-1	5uM(F/c)	3.85×10^6	10^4	77
	340-2	10uM(F/c)	3.60×10^6	10^4	72
	340-3	20uM(F/c)	3.40×10^6	10^4	68
	340-4	40uM(F/c)	1.25×10^6	10^4	25

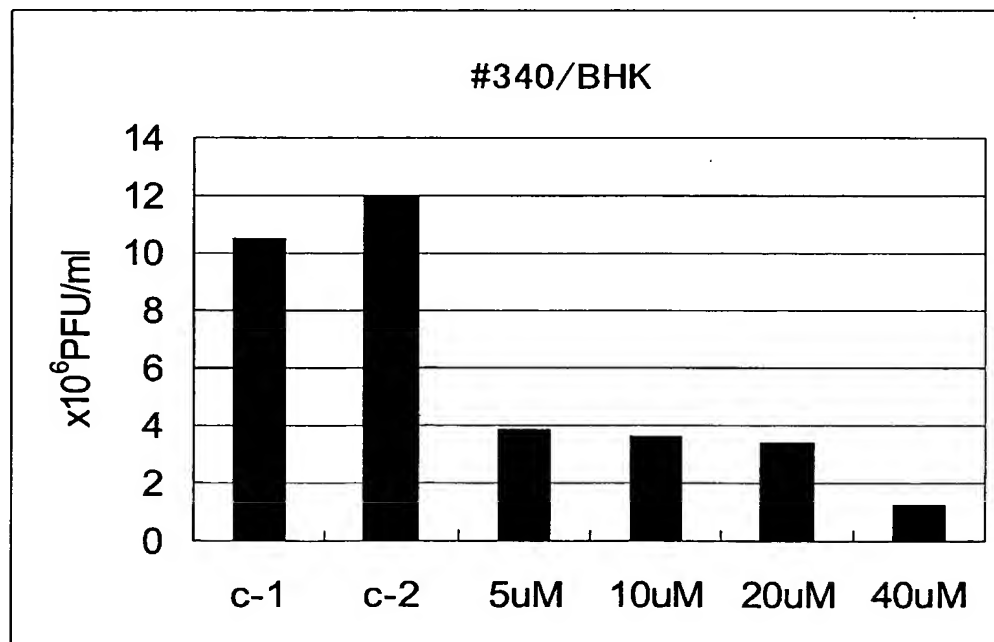

BEST AVAILABLE COPY

FIG. 7

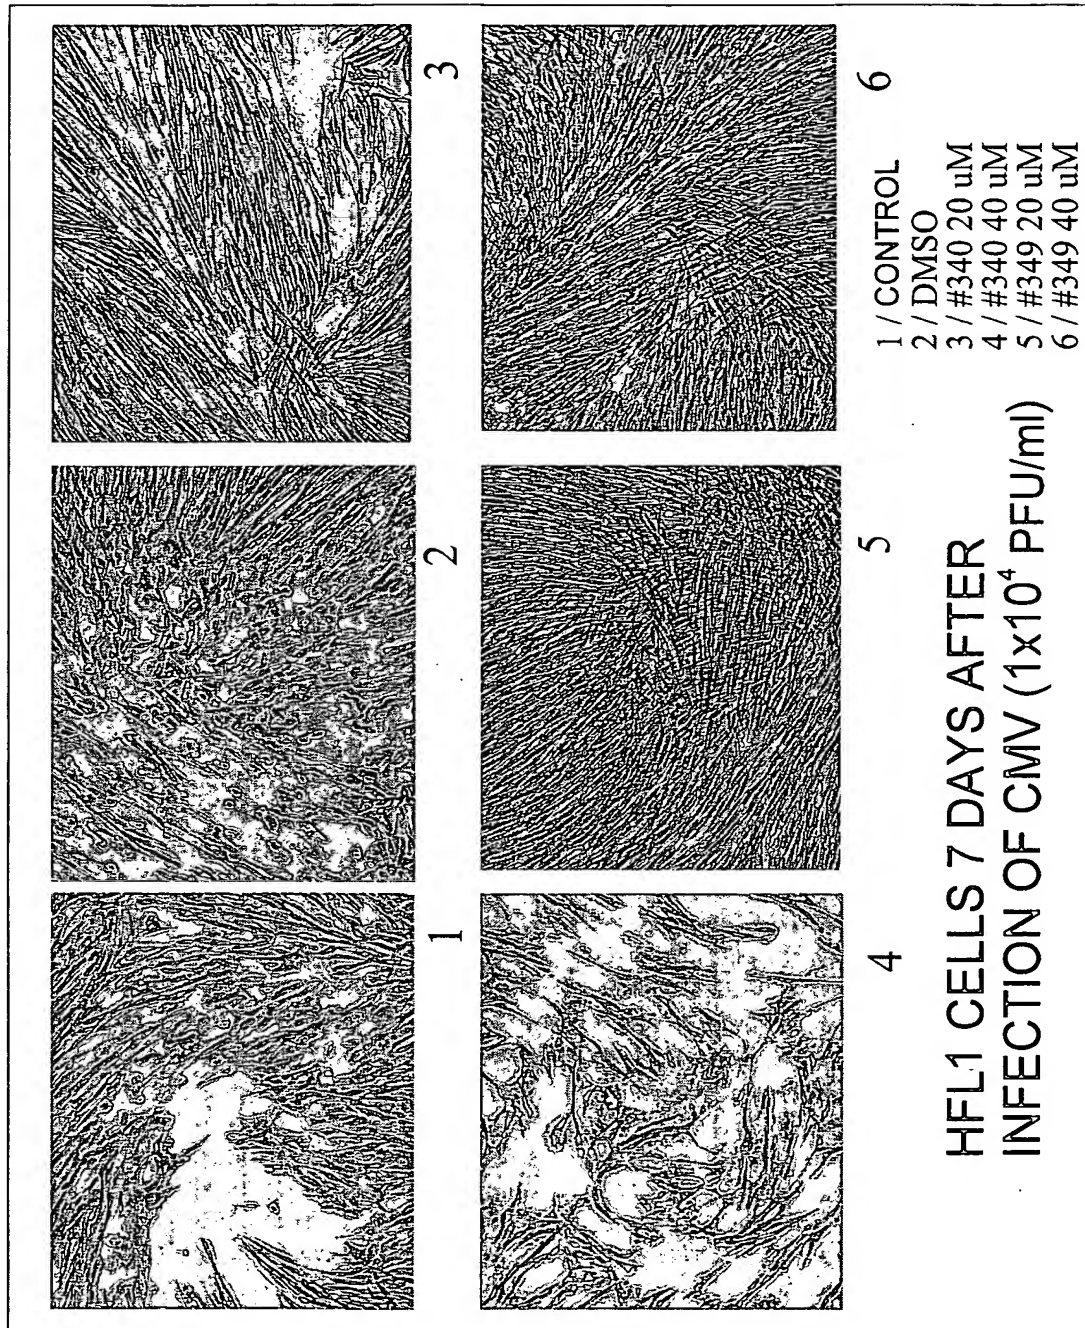


BEST AVAILABLE COPY

FIG. 8

(A)


CONTROL #340 #349
(40 μ M) (40 μ M)

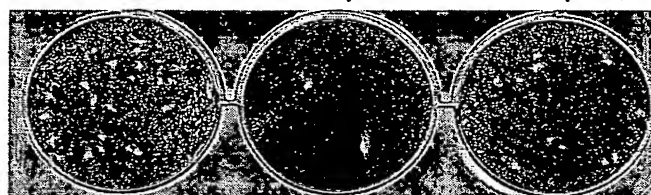

15.5 1.5 7 (*10⁶ PFU/ml)

(B)

C: CONTROL,
S: SRPIN-1(#340) CONCENTRATION (μ M)

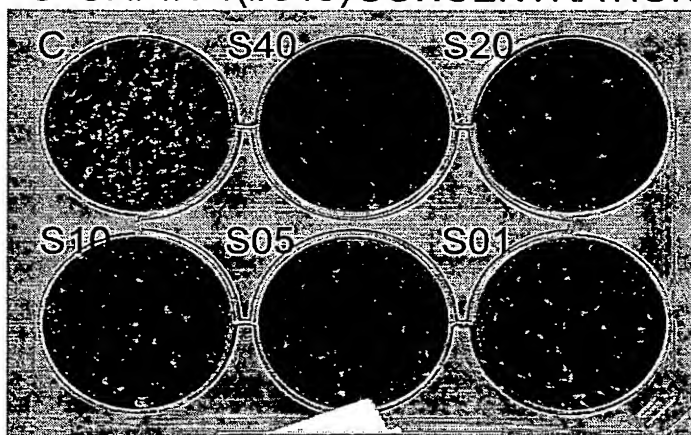

BEST AVAILABLE COPY